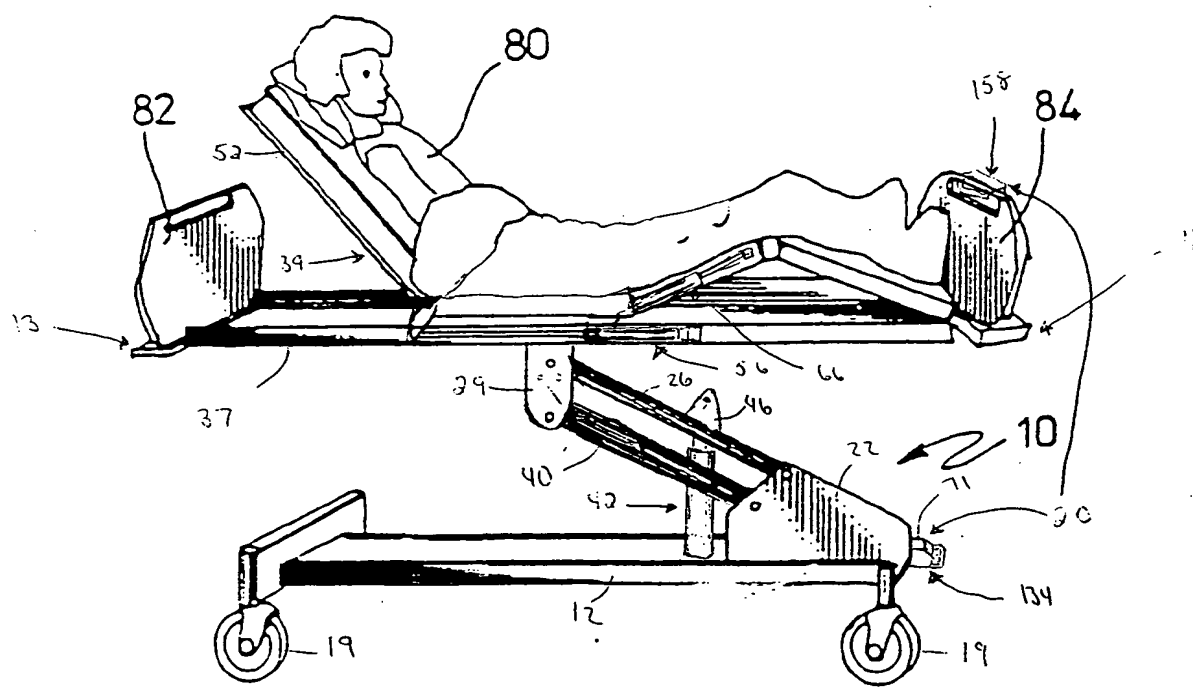
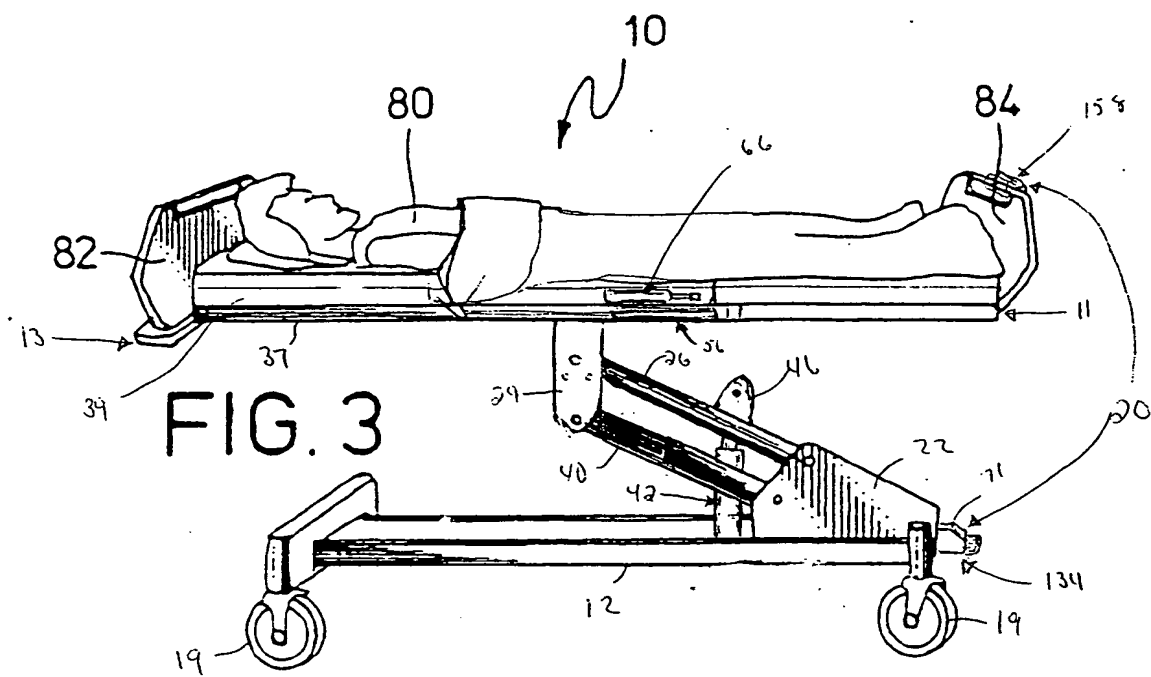


FIG. 1 / 12



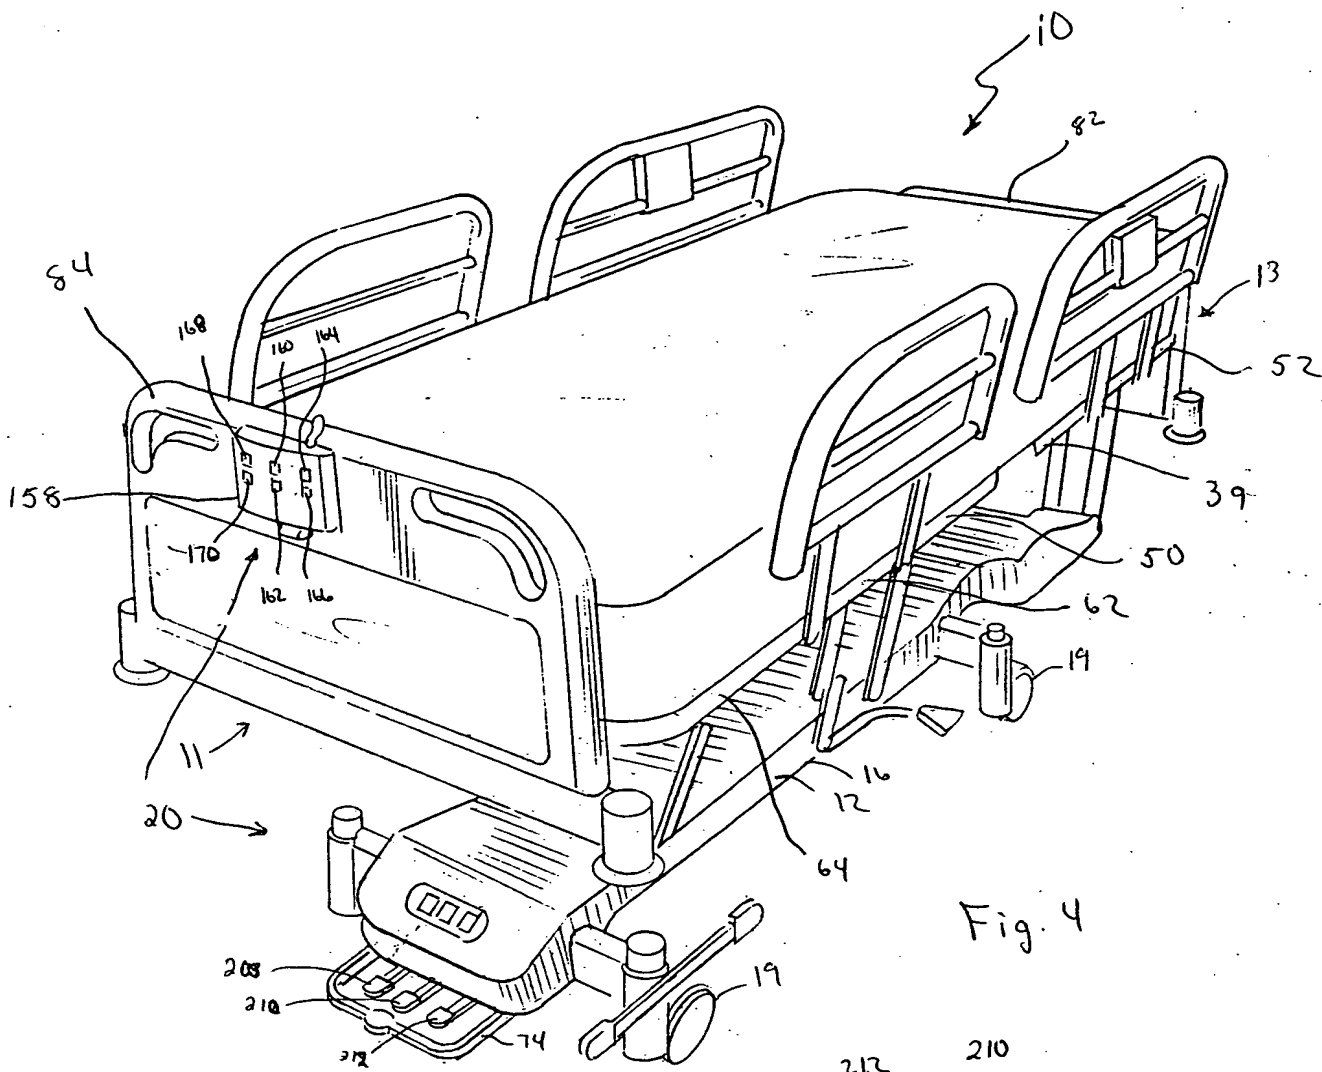


Fig. 4

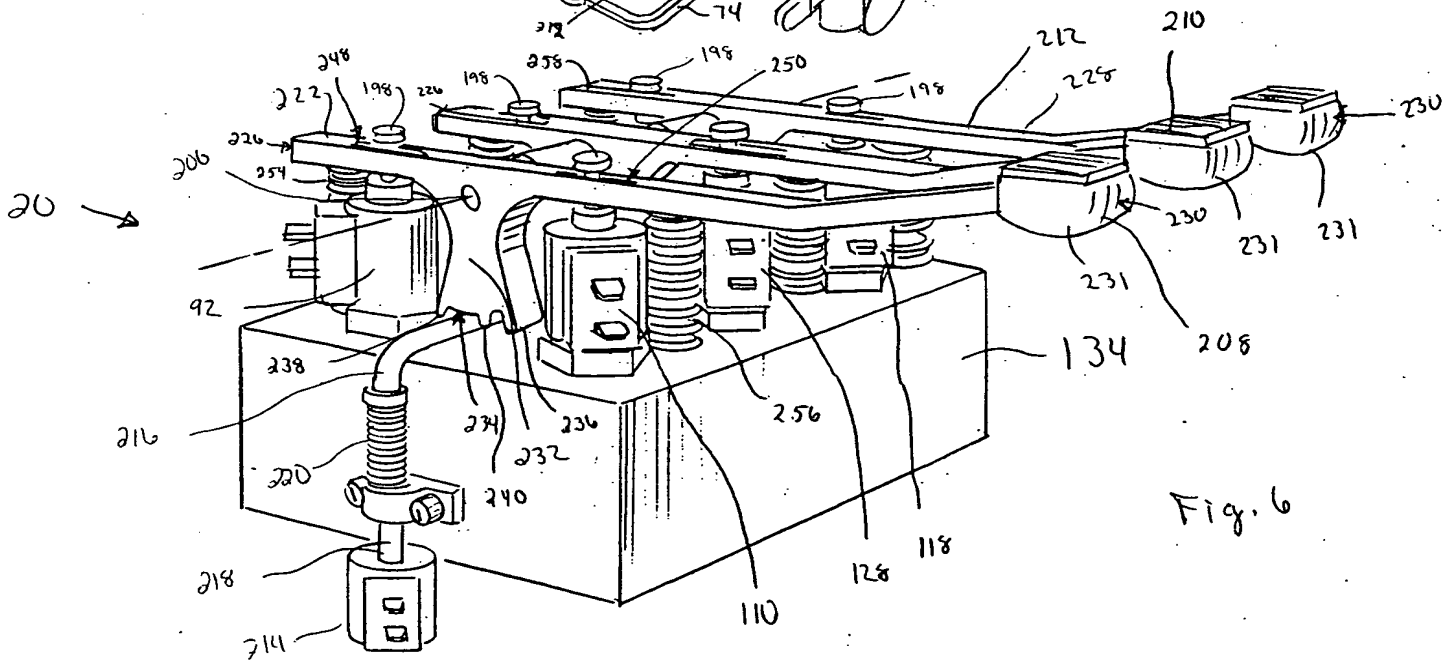


Fig. 6

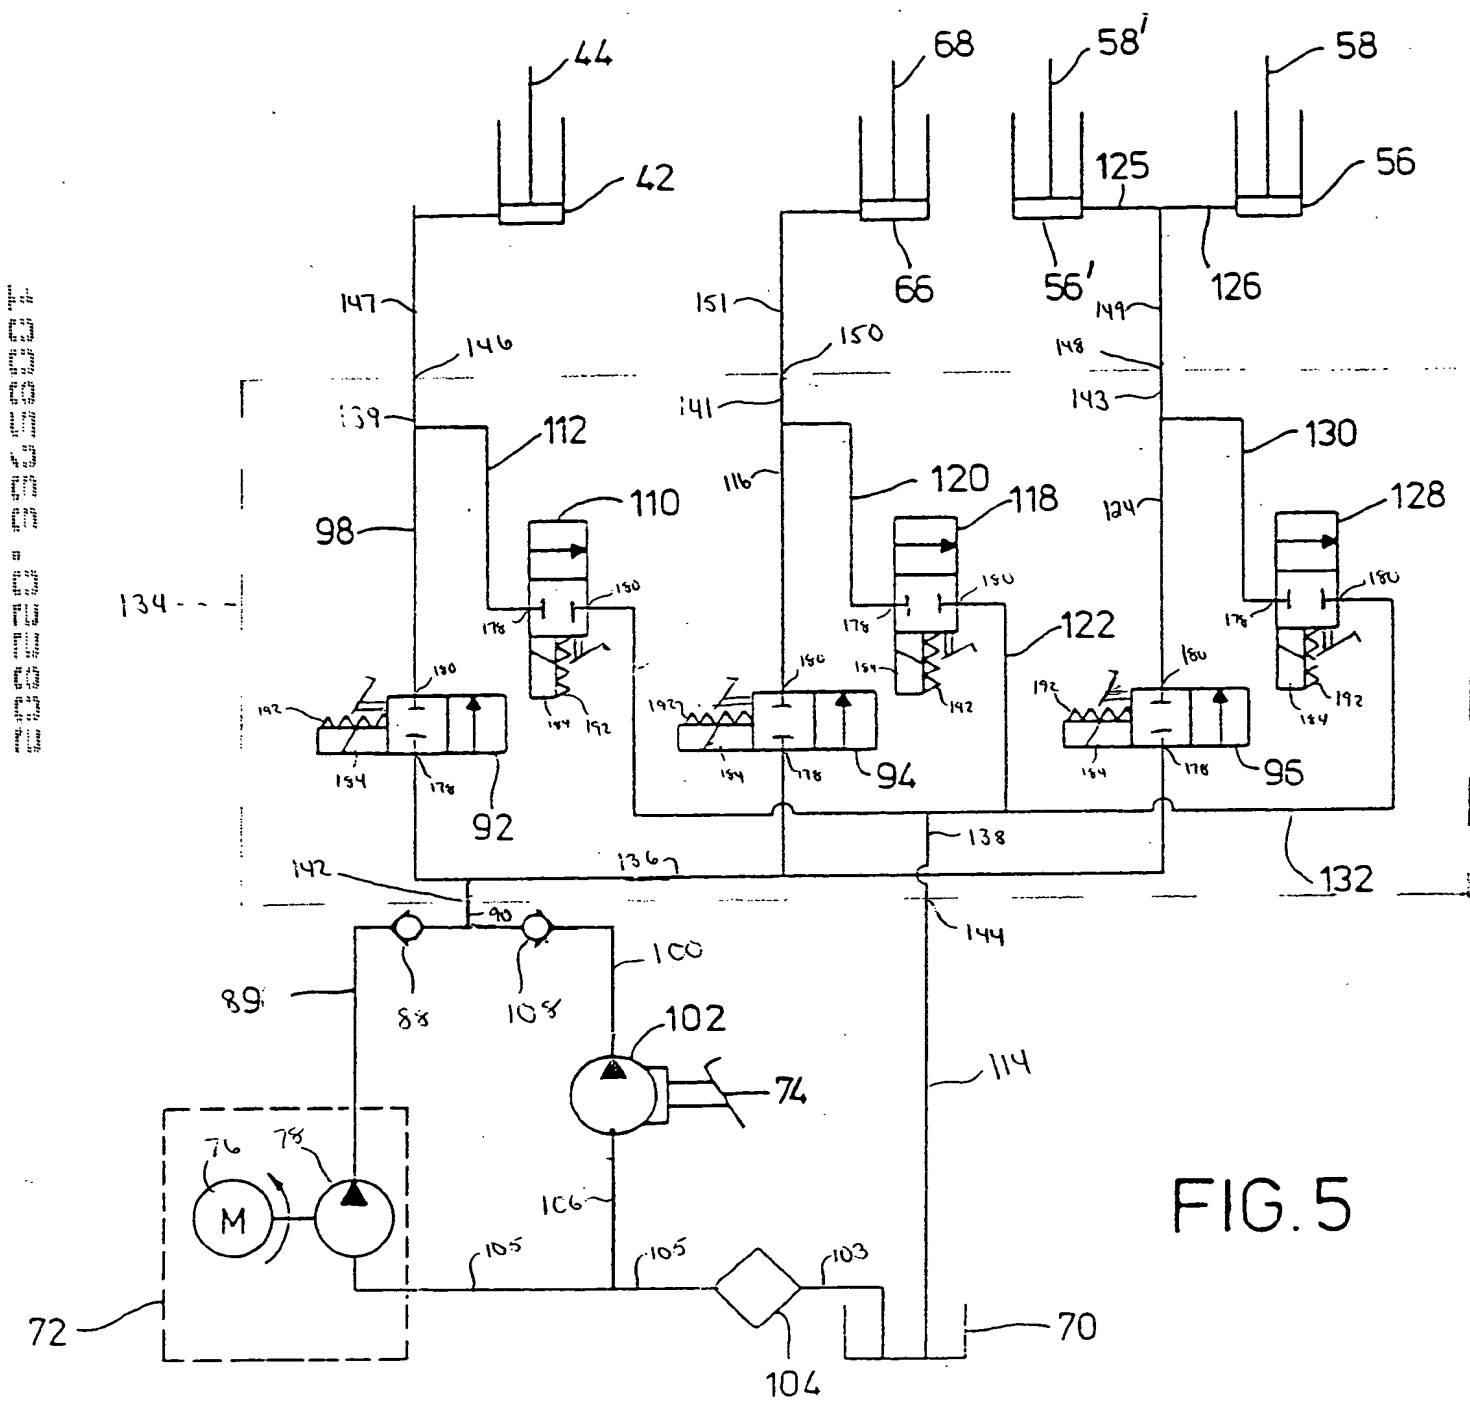


FIG. 5



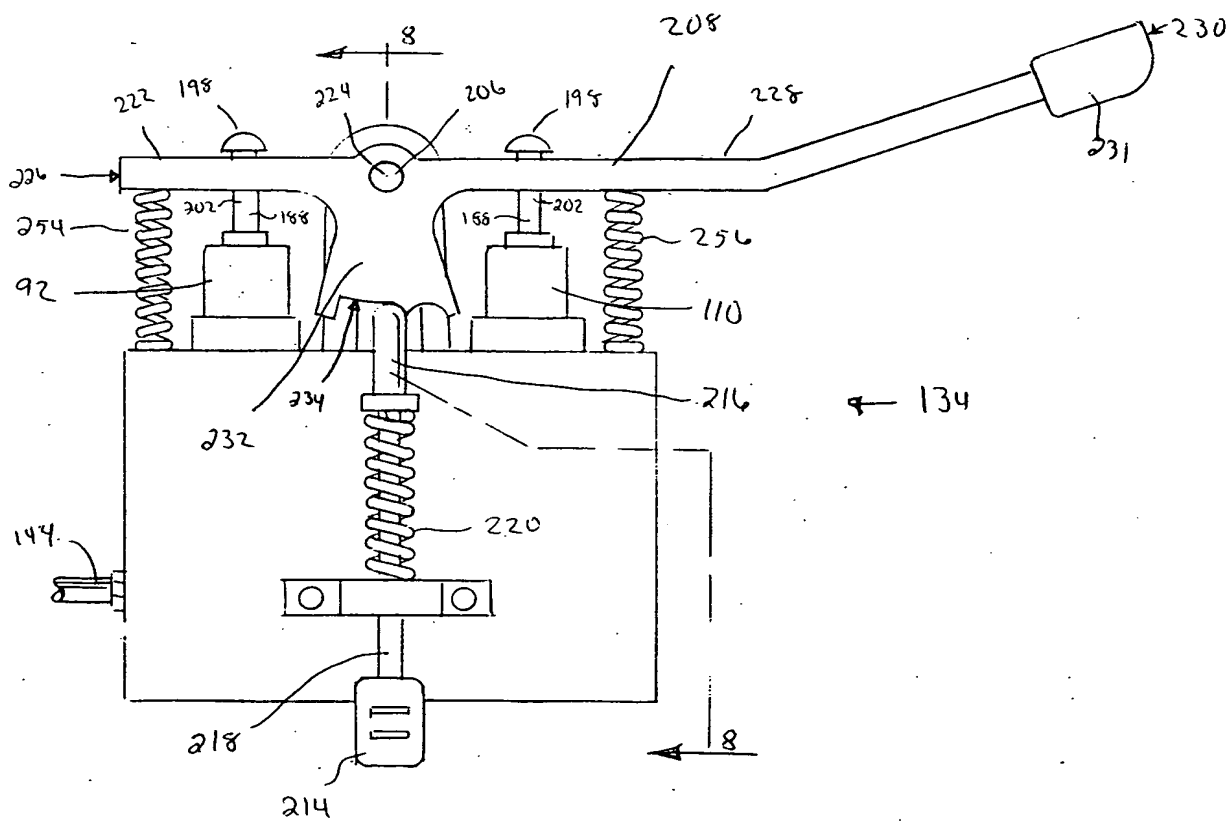


FIG. 9 is a cross-sectional view of the device 20 taken along line 9-9 of FIG. 1.

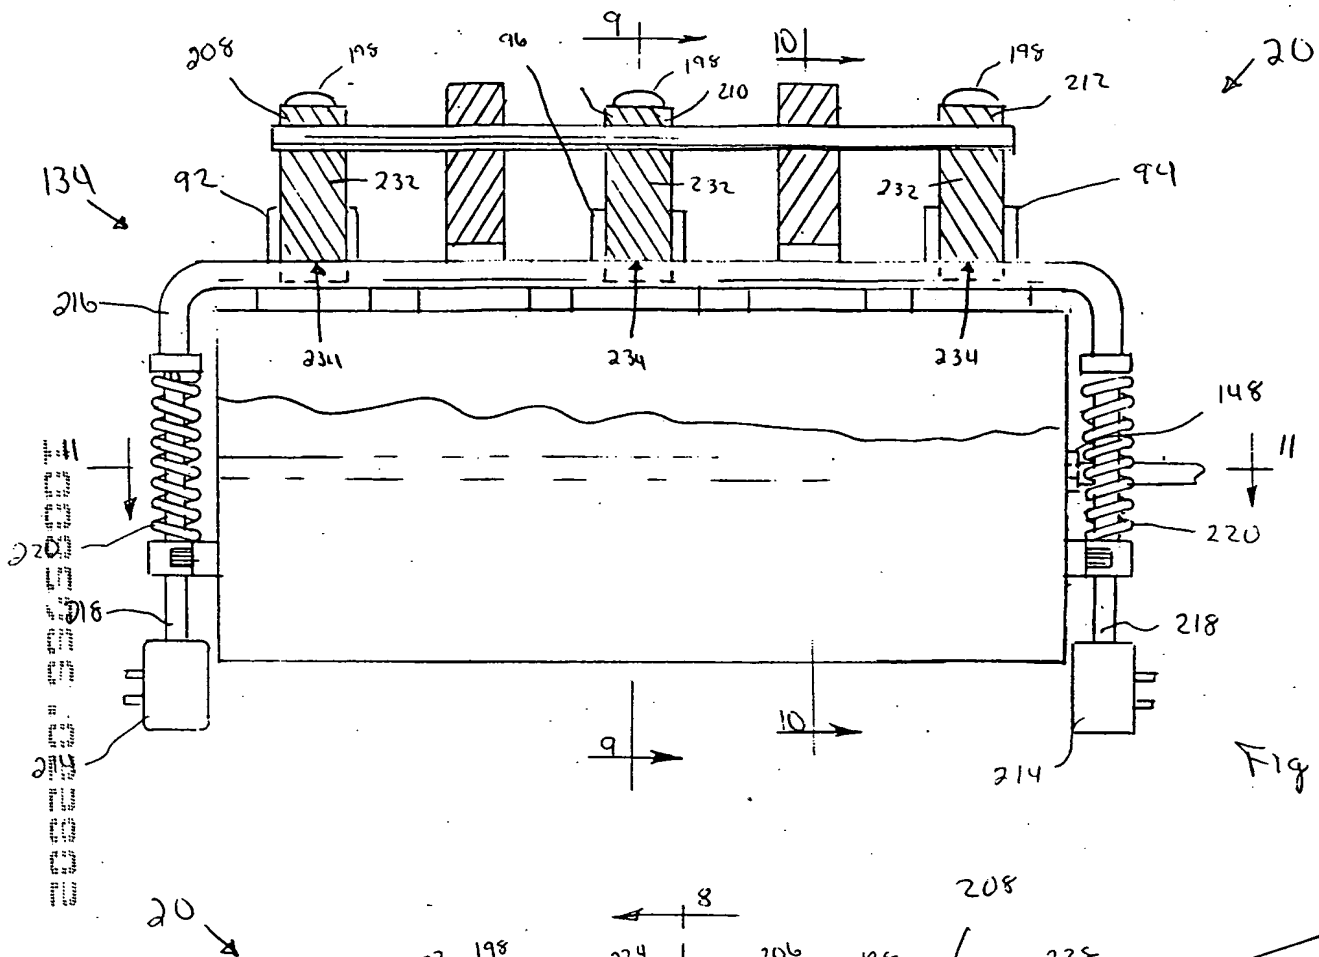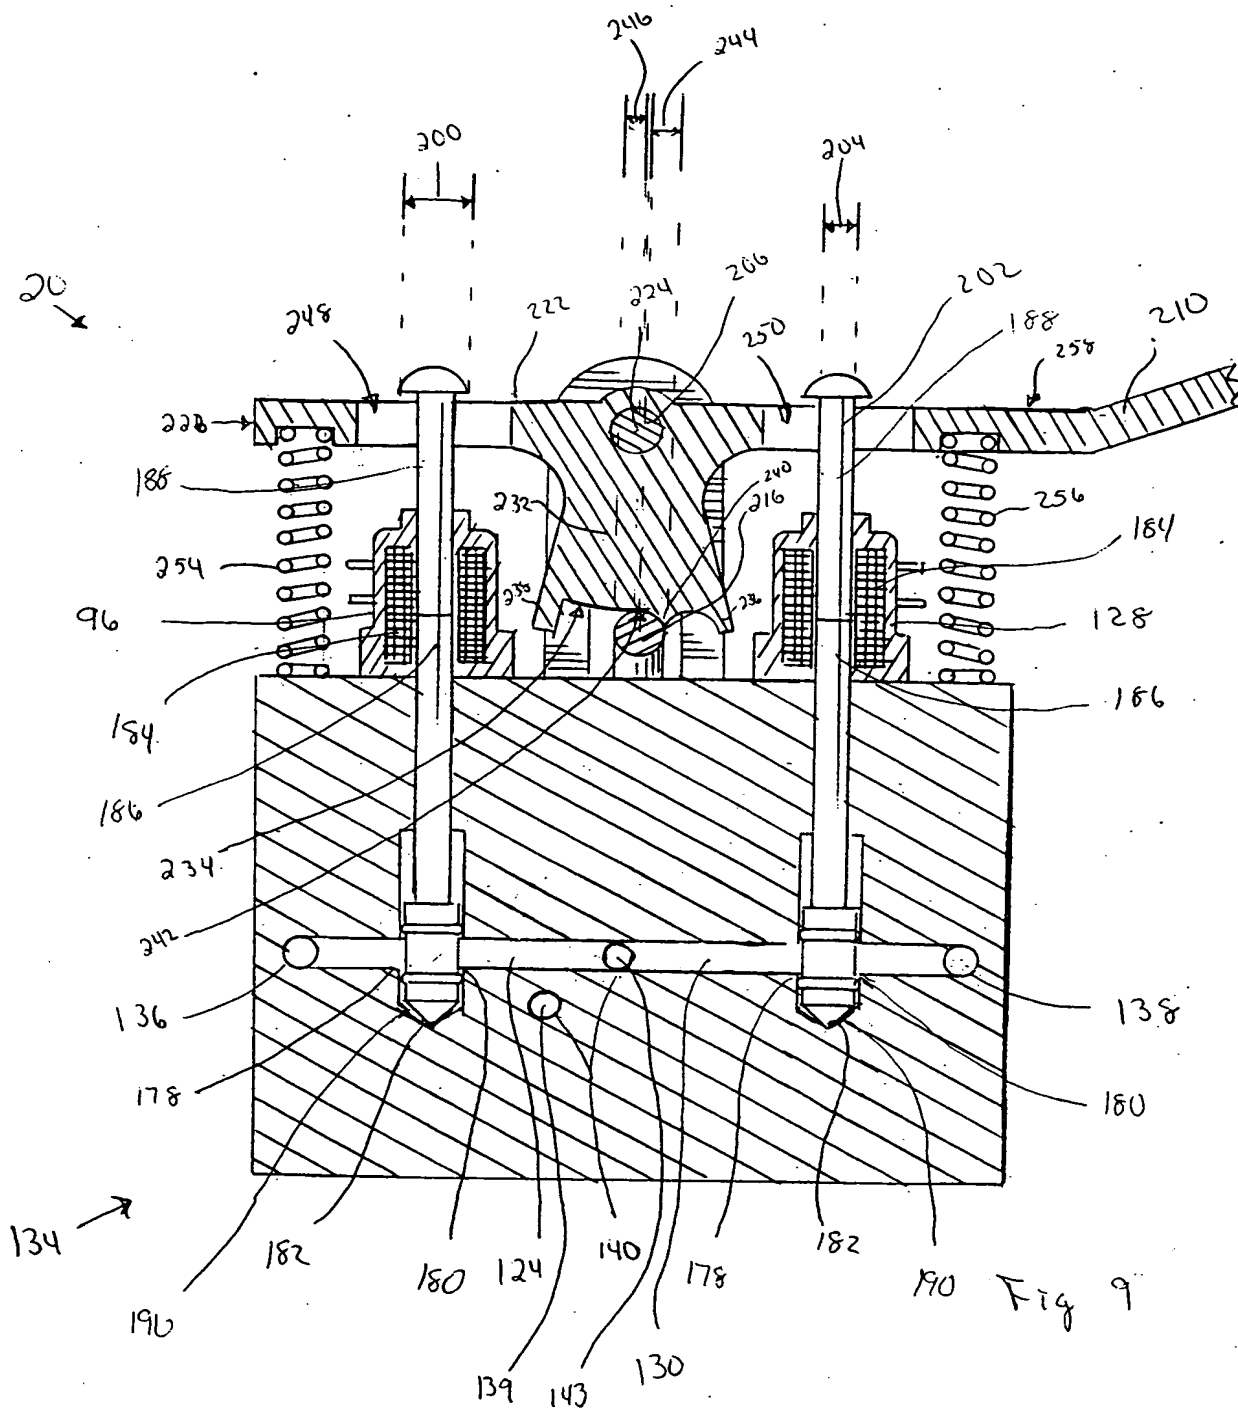

20 x

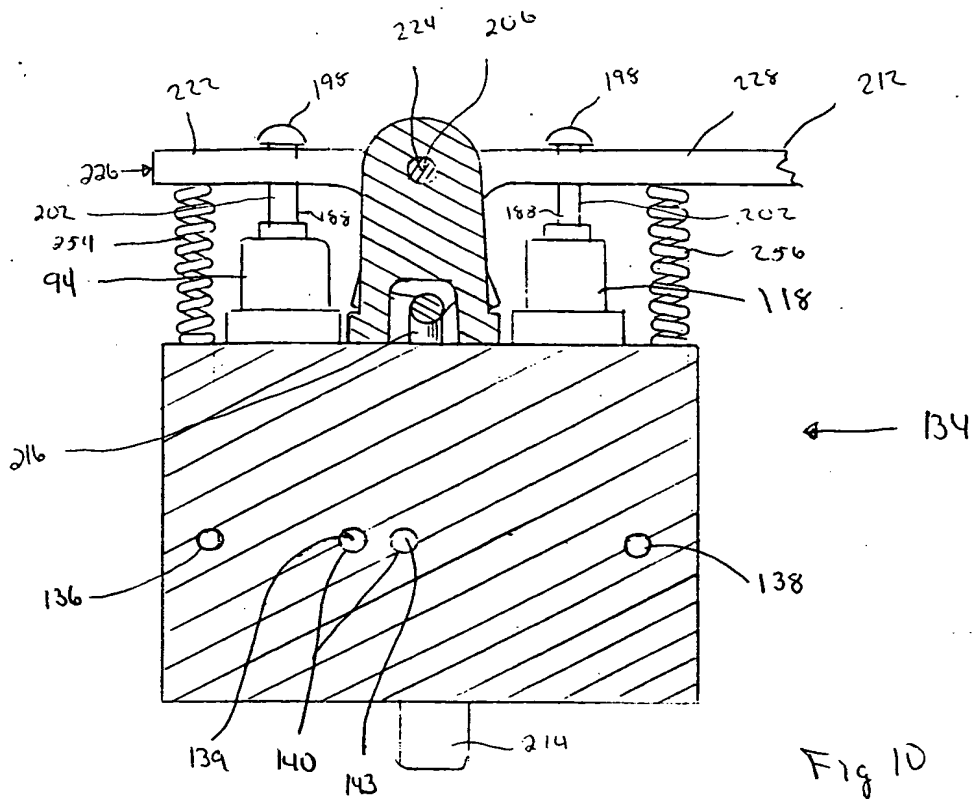


Fig 10

20 x

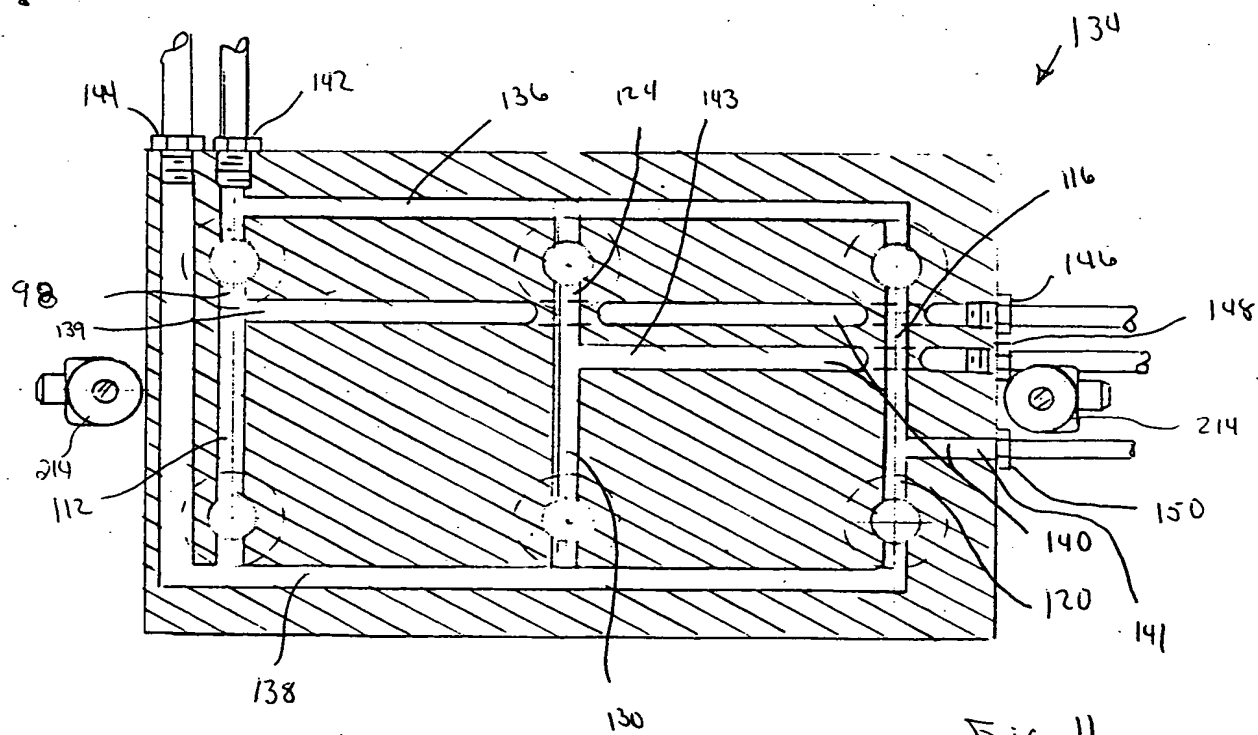


Fig 11

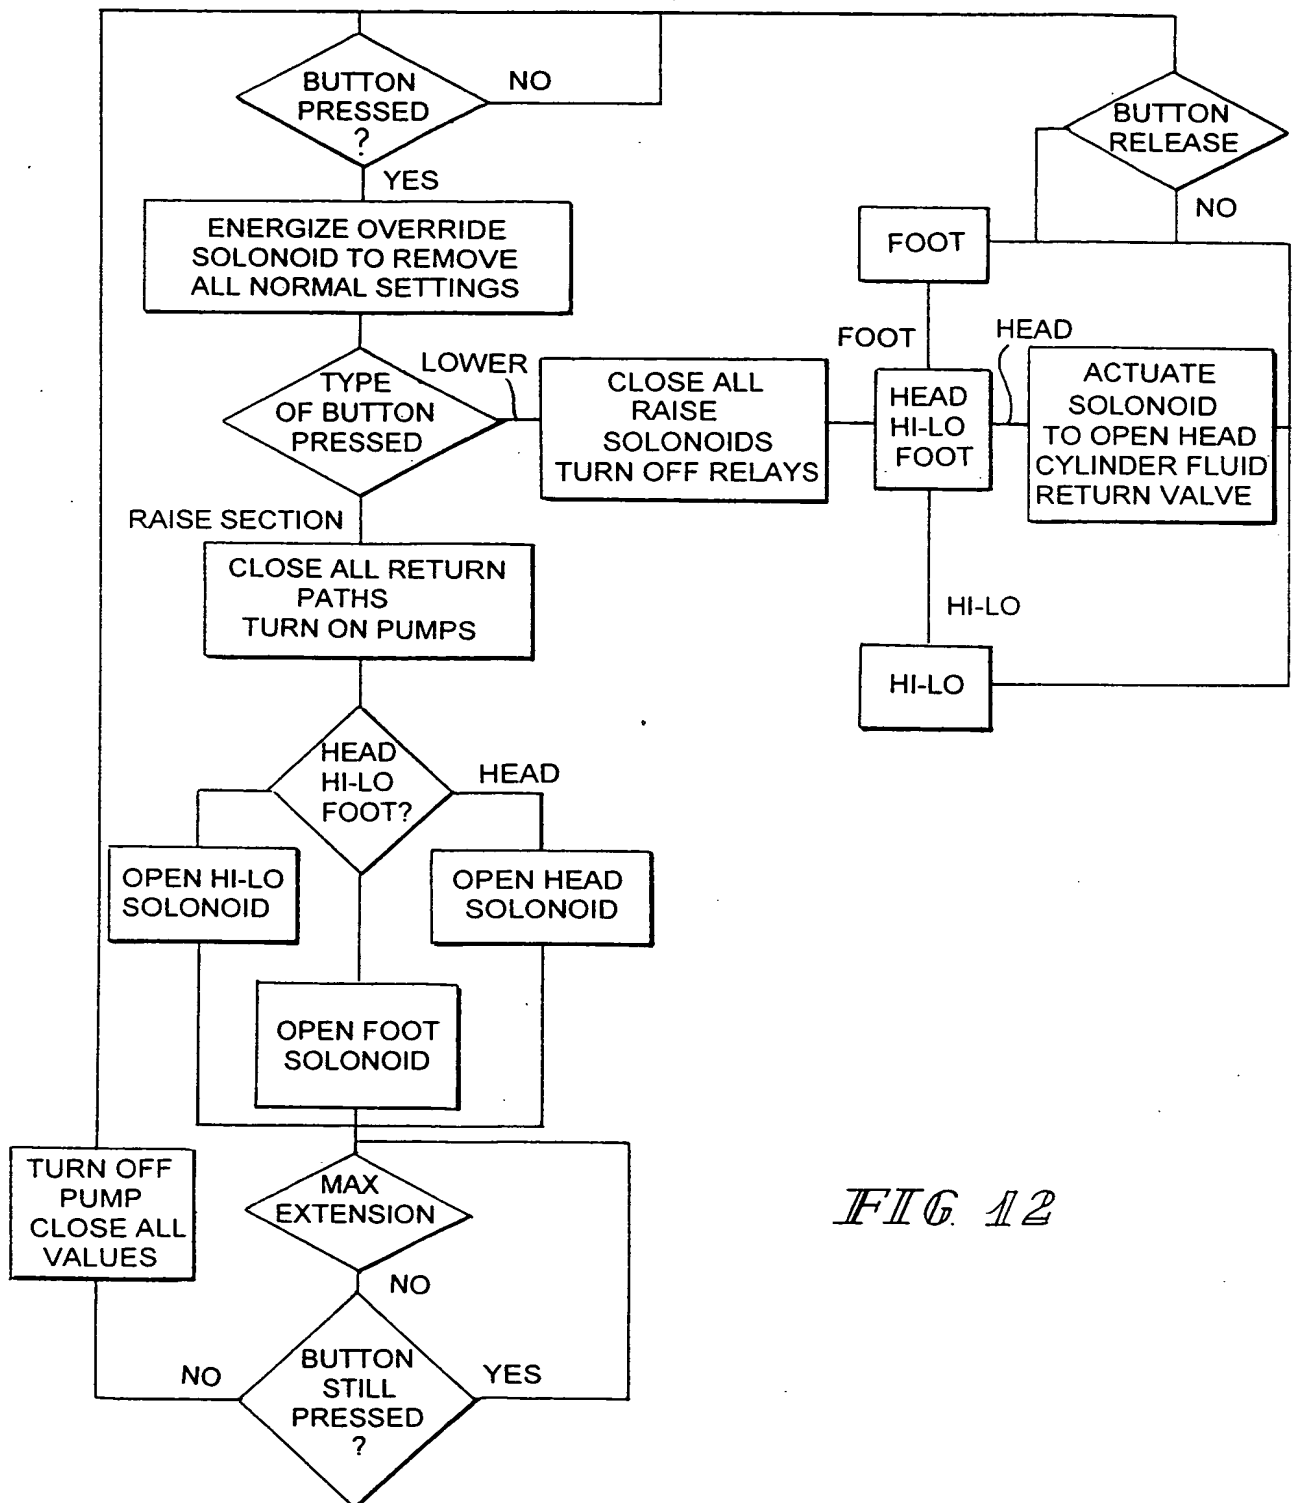


FIG 12



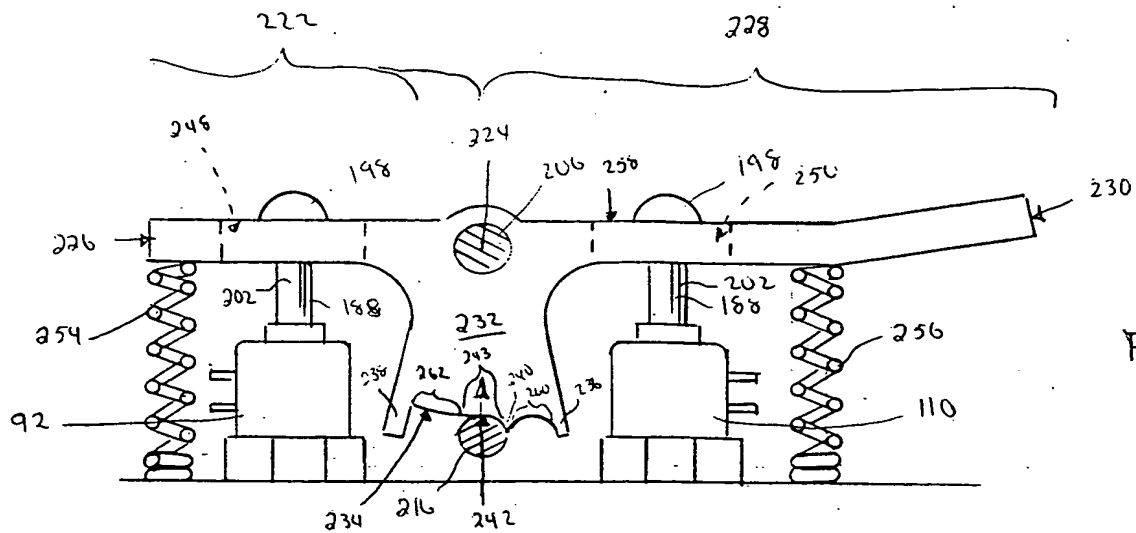


Fig. 13

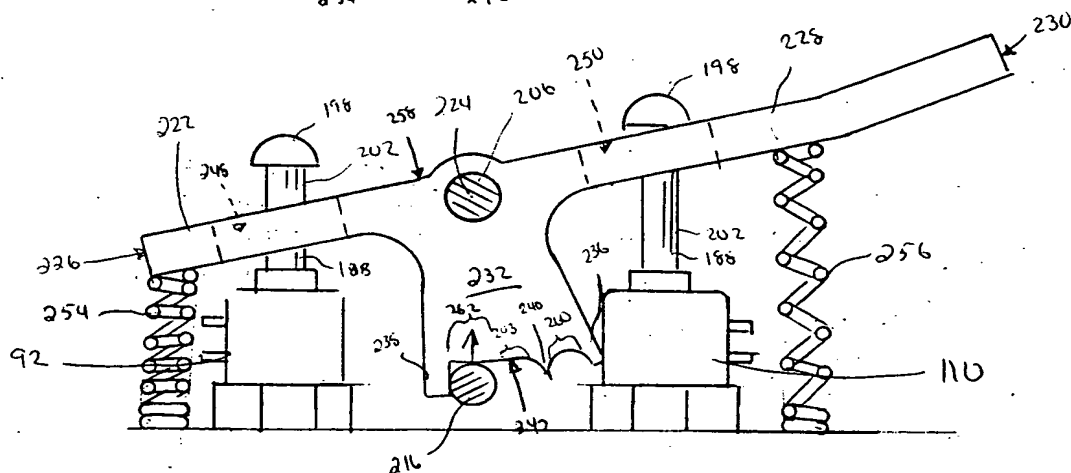


Fig. 14

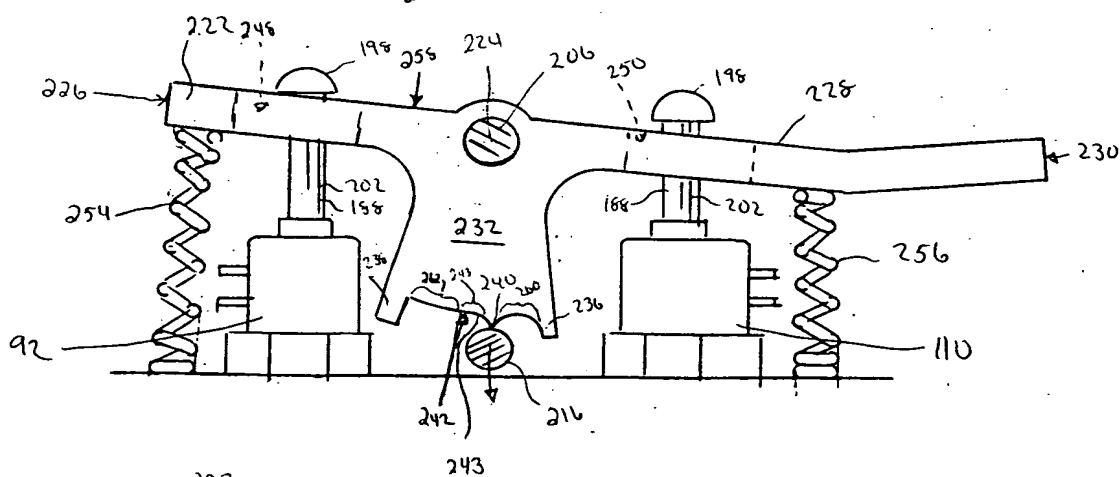


Fig. 15

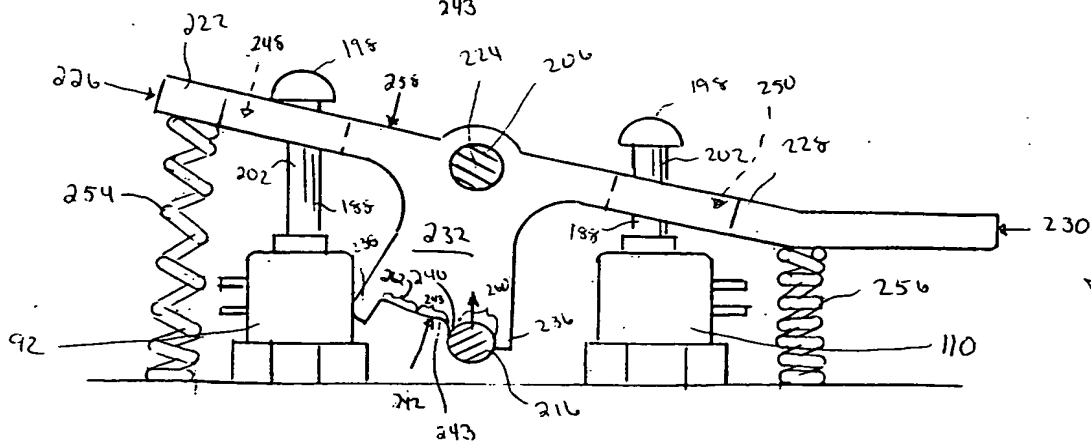


Fig. 16